

2.4. Changing measurement units

ECH2O Utility has a feature that allows changing the measurement units for various parameters. This capability allows data to be downloaded and displayed in the measurement unit of choice for these parameters (Figure 10). To change measurement intervals in ECH2O Utility, follow the steps below.

- Click on the Preferences” tab in the Edit menu.
- Select the units desired for the parameter in question from the options available.

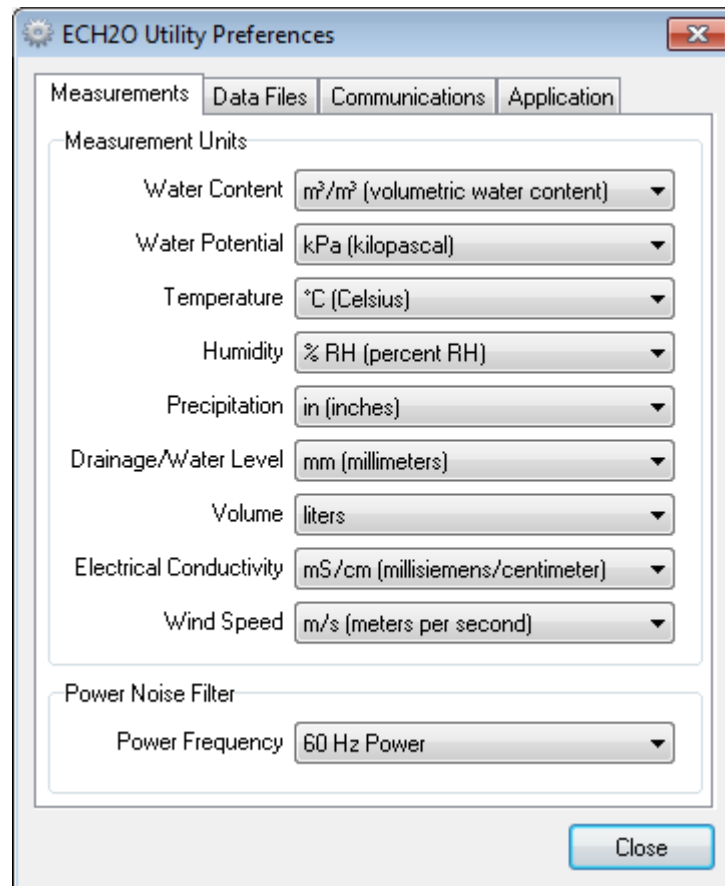


Figure 10. The preference tab in ECH2O Utility showing parameters with more than one unit.